

DOCTOR:

PATIENT:

DATE SENT: _____

DCR CODE: _____ (Compulsory)

AGE: _____ M / F

DATE REQUIRED: AM / PM

Barcode

(O U O L O U&L)

Retainers

- ☐ SmartFit (3D-printed)
- ☐ SmartFit (3D-printed with lingual wire attached)
- ☐ SmartFit (3D-printed with space maintenance)
- ☐ Ecodont Combi (With lingual wire attached)
- ☐ MaX (Zendura) ☐ MaX Lite (Zendura alike)
- ☐ Invisible / Clear ☐ Fixed
- ☐ Hawley ☐ Van der Linden
- ☐ Wrap Around ☐ Begg

Space Maintainers

- ☐ Band & Loop
- ☐ Trans-Palatal Arch (TPA)
- ☐ Lingual Arch
- ☐ Nance Button

Expansion / Arch Development Appliances

- ☐ Quad-Helix
- ☐ Bi-Helix
- ☐ Rapid Palatal Expander (RPE)
 - ☐ Banded
 - ☐ Bonded

Distalising Appliances

- ☐ Pendulum
- ☐ Acrylic Cervical Occipital Anchorage (ACCO)
- ☐ Lip Bumper

Habitual Appliances

- ☐ Tongue Shield (Thumb Crib)

Functional Appliances

- ☐ Twin Block
- ☐ Andresen Activator
- ☐ Bionator
- ☐ Frankel
- ☐ Herbst
- ☐ Activator to Open / Close
- ☐ Half Open / Open Activator
- ☐ Van Beek Activator
- ☐ Activator with Facebow
- ☐ AdvanSync2

Sports Guards

- ☐ Junior (3mm)
- ☐ Standard (5mm)*
- ☐ Senior (6mm)
- ☐ Elite (6mm + soft insert)
- ☐ Professional (6mm + hard insert)

Anti-Snoring Devices

- ☐ 3DS Advance (Nylon)
- ☐ Elastic Mandibular Advancement Appliance (EMA)
- ☐ The Moses Elite
- ☐ The Serene Silensor


Others

- ☐ Dual Layer Night Guard
- ☐ Soft Night Guard (3mm*)
- ☐ Bleaching Tray
- ☐ Study Model
- ☐ TrioClear Impression
- ☐ Remake

Shade:

Splints

- ☐ SmartFit (3D-printed with thick anterior bite)
- ☐ 3DS Protect (Nylon splint)
- ☐ Flat Plane (Occlusal splint)
- ☐ Michigan Splint (Canine rise)
- ☐ Gelb Splint
- ☐ Nociceptive Trigeminal Inhibition (NTI)
- ☐ Kois Deprogrammer
- ☐ Use Clear Relief
(Thermoplastic, MMA/Amine free)**

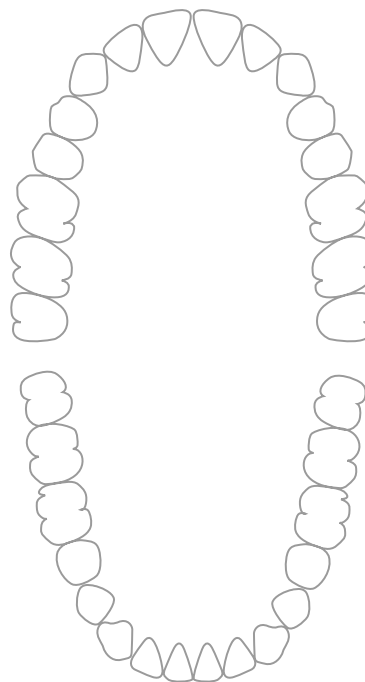

DOCTOR'S INSTRUCTIONS

[illegible]

DOCTOR COPY

* Default protocol will be applied unless specified otherwise
 **Applicable to splints and certain retainers only

Clinic Name & Chop: _____

DOCTOR:

PATIENT:

DATE SENT: _____

DCR CODE: _____ (Compulsory)

AGE: _____ M / F

DATE REQUIRED: AM / PM

BARCODE

(O U O L O U&L)

Retainers

- ☐ SmartFit (3D-printed)
- ☐ SmartFit (3D-printed with lingual wire attached)
- ☐ SmartFit (3D-printed with space maintenance)
- ☐ Ecodont Combi (With lingual wire attached)
- ☐ MaX (Zendura) ☐ MaX Lite (Zendura alike)
- ☐ Invisible / Clear ☐ Fixed
- ☐ Hawley ☐ Van der Linden
- ☐ Wrap Around ☐ Begg

Space Maintainers

- ☐ Band & Loop
- ☐ Trans-Palatal Arch (TPA)
- ☐ Lingual Arch
- ☐ Nance Button

Expansion / Arch Development Appliances

- ☐ Quad-Helix
- ☐ Bi-Helix
- ☐ Rapid Palatal Expander (RPE)
- ☐ Banded ☐ Bonded

Distalising Appliances

- ☐ Pendulum
- ☐ Acrylic Cervical Occipital Anchorage (ACCO)
- ☐ Lip Bumper

Habitual Appliances

- ☐
- Tongue Shield (Thumb Crib)

Functional Appliances

- ☐ Twin Block
- ☐ Andresen Activator
- ☐ Bionator
- ☐ Frankel
- ☐ Herbst
- ☐ Activator to Open / Close
- ☐ Half Open / Open Activator
- ☐ Van Beek Activator
- ☐ Activator with Facebow
- ☐ AdvanSync2

Sports Guards

- ☐ Junior (3mm)
- ☐ Standard (5mm)*
- ☐ Senior (6mm)
- ☐ Elite (6mm + soft insert)
- ☐ Professional (6mm + hard insert)

Anti-Snoring Devices

- ☐ 3DS Advance (Nylon)
- ☐ Elastic Mandibular Advancement Appliance (EMA)
- ☐ The Moses Elite
- ☐ The Serene Silensor


Others

- ☐ Dual Layer Night Guard
- ☐ Soft Night Guard (3mm*)
- ☐ Bleaching Tray
- ☐ Study Model
- ☐ TrioClear Impression
- ☐ Remake

Shade:

Splints

- ☐ SmartFit (3D-printed with thick anterior bite)
- ☐ 3DS Protect (Nylon splint)
- ☐ Flat Plane (Occlusal splint)
- ☐ Michigan Splint (Canine rise)
- ☐ Gelb Splint
- ☐ Nociceptive Trigeminal Inhibition (NTI)
- ☐ Kois Deprogrammer
- ☐ Use Clear Relief
(Thermoplastic, MMA/Amine free)**

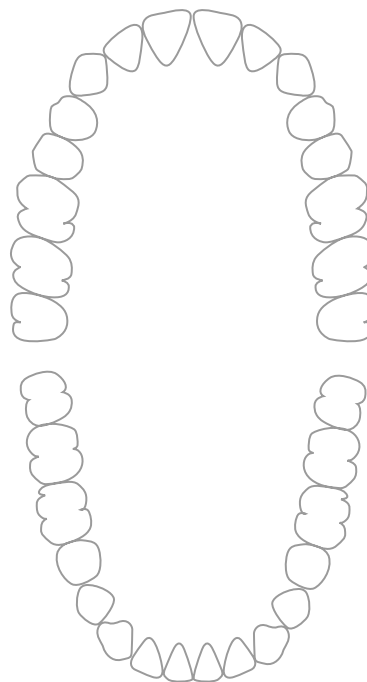

DOCTOR'S INSTRUCTIONS

[illegible]

LAB COPY

* Default protocol will be applied unless specified otherwise
**Applicable to splints and certain retainers only

Clinic Name & Chop: _____

DOCTOR:

PATIENT:

DATE SENT: _____

DCR CODE: _____ (Compulsory)

AGE: _____ M / F

DATE REQUIRED: AM / PM

BARCODE

(O U O L O U&L)

Retainers

- ☐ SmartFit (3D-printed)
- ☐ SmartFit (3D-printed with lingual wire attached)
- ☐ SmartFit (3D-printed with space maintenance)
- ☐ Ecodont Combi (With lingual wire attached)
- ☐ MaX (Zendura) ☐ MaX Lite (Zendura alike)
- ☐ Invisible / Clear ☐ Fixed
- ☐ Hawley ☐ Van der Linden
- ☐ Wrap Around ☐ Begg

Space Maintainers

- ☐ Band & Loop
- ☐ Trans-Palatal Arch (TPA)
- ☐ Lingual Arch
- ☐ Nance Button

Expansion / Arch Development Appliances

- ☐ Quad-Helix
- ☐ Bi-Helix
- ☐ Rapid Palatal Expander (RPE)
- ☐ Banded ☐ Bonded

Distalising Appliances

- ☐ Pendulum
- ☐ Acrylic Cervical Occipital Anchorage (ACCO)
- ☐ Lip Bumper

Habitual Appliances

- ☐
- Tongue Shield (Thumb Crib)

Functional Appliances

- ☐ Twin Block
- ☐ Andresen Activator
- ☐ Bionator
- ☐ Frankel
- ☐ Herbst
- ☐ Activator to Open / Close
- ☐ Half Open / Open Activator
- ☐ Van Beek Activator
- ☐ Activator with Facebow
- ☐ AdvanSync2

Sports Guards

- ☐ Junior (3mm)
- ☐ Standard (5mm)*
- ☐ Senior (6mm)
- ☐ Elite (6mm + soft insert)
- ☐ Professional (6mm + hard insert)

Anti-Snoring Devices

- ☐ 3DS Advance (Nylon)
- ☐ Elastic Mandibular Advancement Appliance (EMA)
- ☐ The Moses Elite
- ☐ The Serene Silensor


Others

- ☐ Dual Layer Night Guard
- ☐ Soft Night Guard (3mm*)
- ☐ Bleaching Tray
- ☐ Study Model
- ☐ TrioClear Impression
- ☐ Remake

Shade:

Splints

- ☐ SmartFit (3D-printed with thick anterior bite)
 - ☐ 3DS Protect (Nylon splint)
 - ☐ Flat Plane (Occlusal splint)
 - ☐ Michigan Splint (Canine rise)
 - ☐ Gelb Splint
 - ☐ Nociceptive Trigeminal Inhibition (NTI)
 - ☐ Kois Deprogrammer
 - ☐ Use Clear Relief
- (Thermoplastic, MMA/Amine free)**

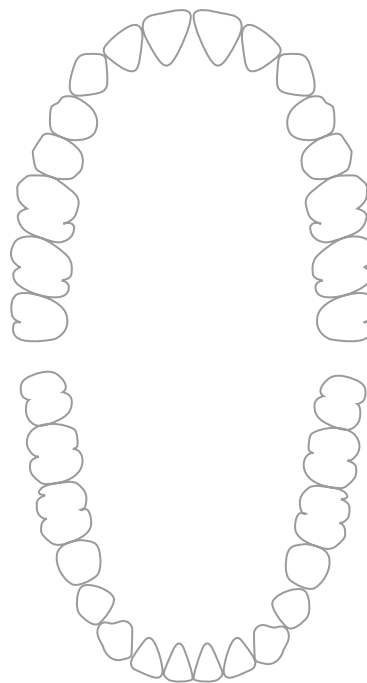

DOCTOR'S INSTRUCTIONS

[illegible]

MDL COPY

* Default protocol will be applied unless specified otherwise
**Applicable to splints and certain retainers only

Clinic Name & Chop: _____